

TECHNE

Sample Concentrator

OPERATOR'S MANUAL

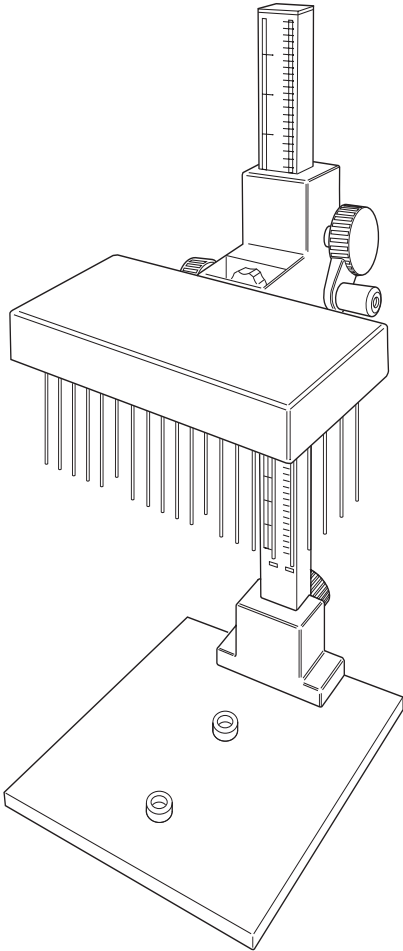

CONTENTS

	PAGE
INTRODUCTION	2
Warning	2
Operator safety	3
Specification	3
Installation	3
Diagram of Sample Concentrator	4
Guarantee	5
OPERATION	6
Preparation	7
Operation	8
ADDITIONAL INFORMATION	9
User maintenance	9
Solvent evaporation temperatures	10
Diagram of gas chamber	12
Replacement parts	13

INTRODUCTION

Please read all the information in this user manual before using the Sample Concentrator.

The Techne Sample Concentrator has been designed to provide a quick and convenient method of accelerating the concentration by evaporation of solvents from samples prior to analysis. It is designed to work in conjunction with Techne DB100/3, DB200/3, DB-3, and DB-3A Dri-Block[®] heaters*.

The Sample Concentrator consists of a gas chamber mounted above a Dri-Block[®] heater into which vessels containing samples are placed. Hyperdermic needles carry the gas down from the chamber into the test tubes. The samples are heated from below by the heater and the flow of gas directed over the surface of the samples displaces the evaporated solvent from above the liquid's surface. This significantly increases the rate of sample concentration.

The unit provides accurate and reproducible control over the positioning of the needles. The gas chamber can be removed from its stand to provide easy access to the samples, and it can be replaced quickly. The whole unit is compact enough for convenient use in a fume cupboard.

WARNING

HIGH TEMPERATURES ARE DANGEROUS: they can cause serious burns and ignite combustible material. Users should pay attention to the following points:

- USE CARE AND WEAR PROTECTIVE GLOVES TO PROTECT HANDS;
- DO NOT put hot objects on or near combustible objects;
- DO NOT place any liquid directly into your Dri-Block[®] heater;
- At all times USE COMMON SENSE.

**The Dri-Block[®] heater is not provided and must be purchased separately.*

SAFETY ADVICE BEFORE USE

OPERATOR SAFETY

All users of Techne equipment must have available the relevant literature needed to ensure their safety.

It is important that only suitably instructed personnel operate this equipment, in accordance with the instructions contained in this manual and with proper safety standards and procedures.

SPECIFICATION


Maximum vertical travel	320 mm
Maximum gas pressure	2 psi
Maximum gas usage	15 litres/min
Gas	Any inert gas (often nitrogen)
Needle positions	Variable to suit Techne Dri-Blocks®
Gas Intake Nozzle Diameter	6.35 mm (¼")
Height	530 mm
Width	240 mm
Depth	295 mm
Weight	3.5 Kg

INSTALLATION

For packing purposes the Sample Concentrator is supplied unassembled in three parts; the base board, the column and carriage, and the gas chamber. The unit is re-assembled as follows:

1. Unscrew the column fastening knob from the column support bracket already fixed to the base board. Locate the column on the two pins in the support bracket. Screw the fastening knob through the rear of the column and tighten firmly.
2. Align the threaded hole on the back of the gas chamber with the mounting on the carriage. Tighten the locking knob to secure the gas chamber in position.

DIAGRAM OF SAMPLE CONCENTRATOR

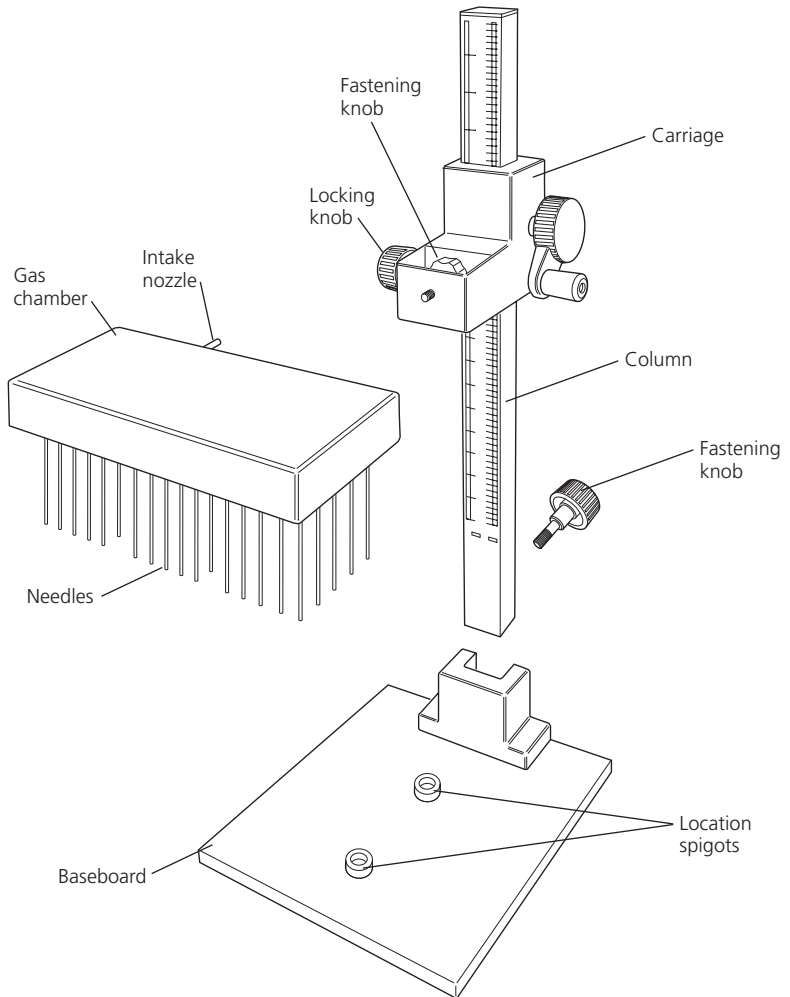

3. Connect the intake nozzle at the rear of the gas chamber to a suitable supply of gas via a pressure reducing valve. The gas pressure should be adjusted as required at the reducing valve but should not exceed 2 psi. Pressure in excess of 2 psi will cause gas to be vented and wasted.
4. Place the Techne Dri-Block[®] heater onto the base of the Sample Concentrator. It is positioned by means of two spigots on the base board which align with two centrally located screw heads on the underside of the Dri-Block[®] unit.

GUARANTEE

This instrument is guaranteed against any defect in material or workmanship for a period as specified on the enclosed guarantee card. This period is from the date of purchase, and within this period all defective parts will be replaced free of charge provided that the defect is not the result of misuse, accident or negligence. Servicing under this guarantee should be obtained from the supplier.

Notwithstanding the description and specification(s) of the units contained in the user manual, Techne hereby reserves the right to make such changes as it shall see fit to the units or to any component of the units.

This user's manual has been prepared solely for the convenience of Techne customers and nothing in this manual shall be taken as a warranty, condition or representation concerning the description, merchantability, fitness for purpose or otherwise of the units or the components.

OPERATION


Preparation


1. Place the aluminium insert blocks to be used into the Dri-Block® unit. The blocks should touch each other and be positioned centrally.
2. Loosen the locking knob on the carriage. Remove the gas chamber, disconnecting the gas pipe if necessary, and lay the chamber upside down on a suitable work surface.
3. Insert the hyperdermic needles in the pattern to suit the test tubes to be placed in the heater.

The needle guide holes are labelled with a letter corresponding with the type of insert block used in the heater. These are listed in the following table. As an example if you use the block for twelve 15mm test tubes (e.g. block number F3506) you would place a needle in all the holes labelled C.


Only Sample Concentrators with the part number FSC496D or a replacement head part number 6106467 will have the 96 well array.

<i>Tube size & diameter</i>	<i>Hole array</i>	<i>Hole label</i>
5 x 6 deep	30	A
4 x 5 deep	20	B
3 x 4 deep	12	C
8 hole off-set array, e.g. F4490		D



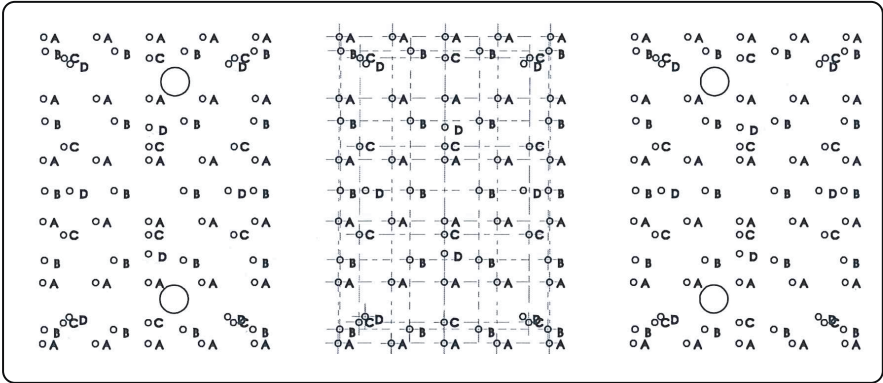


FSC400D matrix plate

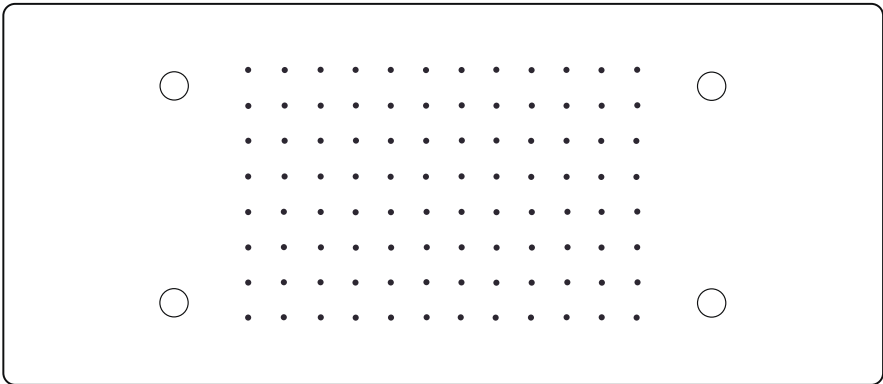

FSC496D matrix plate

Press each needle firmly, pointed end first, through the guide holes and through the sealing pad behind so that it is held firmly in position. Build up the desired pattern of needles to suit the arrangement of test tubes to be used. Do not put a needle in any position which will not have a corresponding sample to be concentrated as this will only waste gas. The needles may be removed and replaced many times as the pad is self sealing.

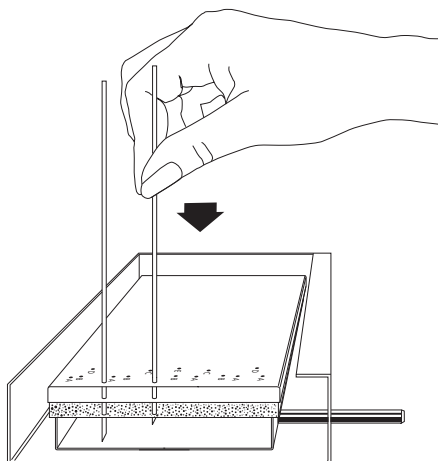

INSERTING THE NEEDLES

4. Replace the gas chamber onto the carriage and tighten the locking knob. Re-connect the gas pipe if necessary.

PROCESSING OF SAMPLES

Warning - remember high temperatures are dangerous. The heater, insert blocks, sample vessels, needles and samples may be very hot. Always take the precautions listed earlier in this manual.

1. By turning the carriage handle, on the right hand side, counter clockwise raise the gas chamber to take the needles well away from the heater.
2. Place the sample vessels in the insert blocks and lower the chamber so that the tips of the needles enter the test tubes. Position them at the required height above the liquid surface.
3. Set the heater to the required temperature and adjust the gas flow to the desired rate. Remember not to exceed 2 psi.
4. To increase the rate of concentration the chamber may be lowered as evaporation takes place so that the needles follow the level of the samples in the tubes. Using the scale on the column fine adjustments are easily made.
5. On completion switch off the gas flow and raise the chamber out of the way.
6. For operation of the Dri-Block[®] see the user's manual supplied separately.

ADDITIONAL INFORMATION

User maintenance

1. Cleaning

Your Sample Concentrator can be cleaned by wiping with a cloth dipped in soapy water. Ethanol and formaldehyde may also be used. Do not use abrasive cleaners.

2. Carriage friction

Height adjustment is by means of a friction drive. To allow for wear the friction pressure may be increased by tightening the 4 screws on the rear of the carriage sufficiently to give adequate grip. Ensure that all four are tightened equally.

3. To replace the sealing pad

After many repeated needle insertions the self sealing property of the sealing pad may start to degrade. Spare pads can be obtained from your supplier or from Techne. Replacing the pad is simply accomplished as follows:

- Remove the gas chamber from the carriage, disconnect the gas pipe and place upside down on a suitable work surface.
- Remove the four screws securing the matrix plate.
- Lift off the matrix plate.
- Lift off the sealing pad. Ensure that the support strip underneath the sealing pad remains in place.
- Replace the sealing pad with the new one. Reassembly is the reverse of the above procedure.

For any other servicing requirements please contact your supplier or Techne's service department.


SOLVENT EVAPORATION TEMPERATURES

IUPAC Name	Common Name	Boiling point (°C) at 1013 mbar pressure	Pressure (mbar) at which b.p is 40°C
2-propanone	Acetone	56	556
1-pentanol	Pentyl alcohol	137	11
Benzene	Benzene	80	236
1-butanol	Butyl alcohol	118	25
2-methyl-2-propanol	Tert-butyl alcohol	83	130
Chlorobenzene	Chlorobenzene	132	36
Chloroform	Trichloromethane	61	474
Cyclohexane	Cyclohexane	81	235
Ethoxyethane	Diethyl ether	35	Atmospheric
1,2-dichloroethane	Ethylene chloride	83	210
1,2-dichloroethene	Cis-acetylene dichloride	60	479
1,2-dichloroethene	Trans-acetylene dichloride	48	751
2-propan-2-yloxypropane	Isopropyl ether	68	375
1,4-Dioxane	Diethylene oxide	101	107
N,N-dimethylformamide	Dimethylformamide (DMF)	153	11
Acetic acid	Ethanoic acid	118	44
Ethanol	Alcohol	79	175
Ethyl acetate	Ethyl ester	77	40
Heptane	Dipropylmethane	98	120
Hexane	n-hexane	69	335
Propan-2-ol	Isopropanol	82	137
3-methyl-1-butanol	Isoamyl alcohol	130	14
Butan-2-one	Methylethylketone (MEK)	80	243

SOLVENT EVAPORATION TEMPERATURES
continued

IUPAC Name	Common Name	Boiling point (°C) at 1013 mbar pressure	Pressure (mbar) at which b.p is 40°C
Methanol	Methyl alcohol	65	337
Dichloromethane	Methylene chloride	40	Atmospheric
Pentane	Pentane	36	Atmospheric
Propan-1-ol	Propyl alcohol	97	67
1,1,1,2,2-pentachloroethane	Pentachloroethane	162	13
1,1,2,2-tetrachloroethane	Tetrachloroethane	138	35
1,1,1-trichloroethane	Trichloroethane	75	271
Tetrachloromethane	Carbon tetrachloride	76	300
1,1,2,2-tetrachloroethene	Tetrachloroethylene	121	53
Oxolane	Tetrahydrofuran (THF)	67	357
Toluene	Methylbenzene	111	77
1,1,2-trichloroethene	Trichloroethylene	87	183
Oxidane	Water	100	72
Dimethylbenzene	Xylene (mixed)	137	25
1,2-dimethylbenzene	o-xylene	144	34
1,3-dimethylbenzene	m-xylene	139	25
1,4-dimethylbenzene	p-xylene	138	31

DIAGRAM OF GAS CHAMBER

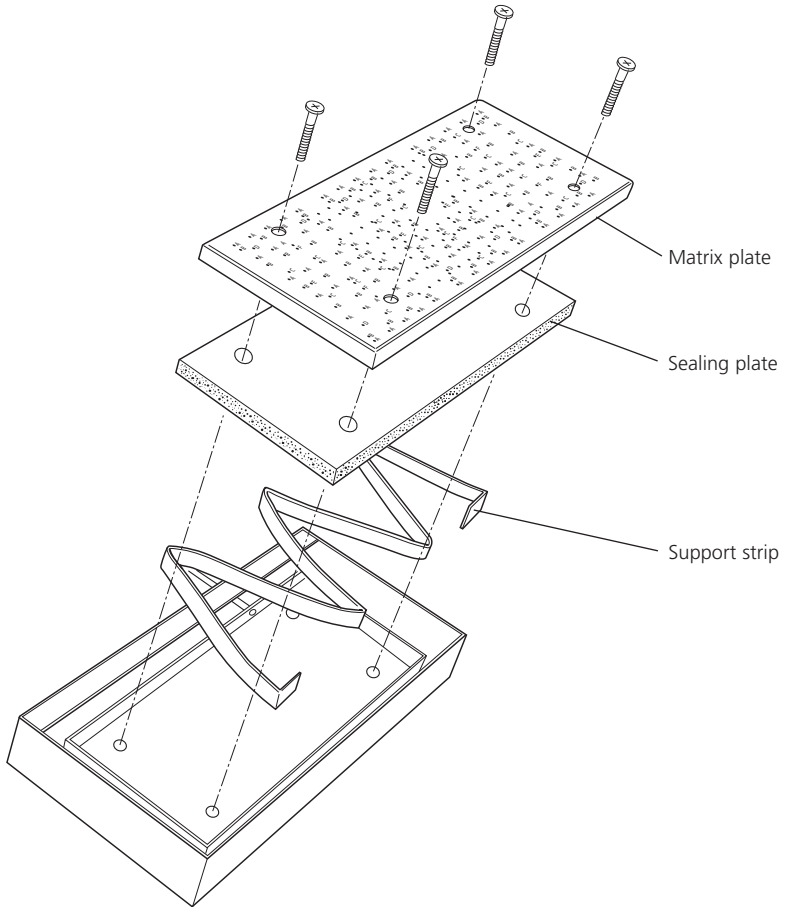

REPLACEMENT PARTS AND ACCESSORIES

The following replacement parts and accessories may be obtained from your supplier or from Techne.

<i>Part Number</i>	<i>Description</i>
F7209	Pack of 100 x 76mm long needles
F7210	Pack of 100 x 127mm long needles
FSC4NCS	Pack of PTFE coated needles, 100 x 76mm long
FSC4NCL	Pack of PTFE coated needles, 100 x 127mm long
6101608	Spigot
6101604	Sealing pad
6101605	Support strip

Spare and alternative heads complete

6106410	Standard, three block, matrix head
6106467	96 well matrix head

Concentrators with various heads

FSC400D	Standard, three block, matrix
FSC496D	96 well matrix



Bibby Scientific - France

Bâtiment le Deltaparc Silic pars Nord 2,
7 rue du Canal,
BP 55437 Villepinte,
95944 ROISSY Charles de Gaulle,
France
Tel: +33 (0) 1 48 63 78 00
Fax: +33 (0) 1 48 63 78 01
Email: contact@bibby-scientific.com
Web: www.bibby-scientific.fr

Bibby Scientific US

3 Terri Lane,
Suite 10,
Burlington,
NJ 08016, USA
Tel: +1 609 589 2560
Fax: +1 609 589 2571
Email: labproducts@techneusa.com
Web: www.bibby-scientific.com

Bibby Scientific UK (Group HQ)

Beacon Road,
Stone,
Staffordshire
United Kingdom ST15 0SA
Tel: +44 (0) 1785 812121
Fax: +44 (0) 1785 810405
Email: sales@bibby-scientific.com
Web: www.bibby-scientific.com

Bibby Scientific - Middle East

PO Box 27842
Engomi 2433,
Nicosia, Cyprus
Tel: +357 22 660 423
Fax: +357 22 660 424
Email: sales@bibby-scientific.me
Web: www.bibby-scientific.com

Bibby Scientific - Singapore

Prudential Tower,
Level 26
30 Cecil Street
Singapore 049712
Tel: + 65 6631 2976
Fax: +44 (0) 1785 810405
Email: info@bibby-scientific.com
Web: www.bibby-scientific.com