

**Genova Nano Spectrophotometer
Micro Volume Accessory**

JENWAY

Accessory Fitting and Operating Manual

Bibby Scientific

737 555 REV B/01-15

Safety

Please read this information carefully prior to installing or using this equipment.

1. The unit described in this manual is designed to be operated only by trained personnel. Any adjustments, maintenance and repair must be carried out as defined in this manual by a person qualified to be aware of the hazards involved.
2. It is essential that both operating and service personnel employ a safe system of work, in addition to the detailed instructions specified in this manual.
3. Other than for those items defined in the maintenance procedures herein, there are no user serviceable items in this instrument. Removal of covers and attempted adjustment or service by unqualified personnel will invalidate the warranty and may incur additional charges for repair.
4. References should always be made to the Health and Safety data supplied with any chemicals used. Generally accepted laboratory procedures for safe handling of chemicals should be employed.
5. If it is suspected that safety protection has been impaired in any way, the unit must be made inoperative and secured against any intended operation. The fault condition should immediately be reported to the appropriate servicing authority.

Merci de lire attentivement ces informations avant d'installer ou d'utiliser cet appareil.

1. L'appareil décrit dans ce manuel est conçu pour être utilisé uniquement par des personnes formées. Tout réglage, maintenance ou réparation doit être effectué comme décrit dans ce manuel, par une personne qualifiée consciente des risques encourus.
2. Il est essentiel que les personnes utilisant et intervenant sur cet appareil respectent les règles de sécurité de travail, en plus des instructions détaillées précisées dans ce manuel.
3. En-dehors des éléments décrits dans les procédures de maintenance ci-incluses, cet appareil ne contient aucun élément réparable par l'utilisateur. L'enlèvement des capots et les tentatives de réglage ou de réparation par des personnes non qualifiées invalide toute garantie et entraîne un risque de frais de réparation supplémentaires.
4. Toujours se référer aux fiches techniques de santé et de sécurité accompagnant tout produit chimique utilisé. Respecter les procédures de laboratoire généralement acceptées pour la manipulation en toute sécurité des produits chimiques.
5. Si l'utilisateur suspecte qu'un problème quelconque puisse mettre en cause la sécurité, l'appareil doit être rendu inopérant en empêchant son utilisation. Communiquer la défaillance constatée au service de maintenance compétent.

Bitte lesen Sie diese Hinweise vor Installation oder Gebrauch dieser Ausrüstung sorgfältig durch.

1. Das in diesem Handbuch beschriebene Gerät darf nur von geschultem Personal bedient werden. Alle Anpassungen, Wartungsarbeiten und Reparaturen müssen entsprechend der Vorgaben in diesem Handbuch und von einer kompetenten Person, die mit den damit verbundenen Gefahren vertraut ist, durchgeführt werden.
2. Es ist wichtig, dass sowohl das Bedienungs- als auch das Service-Personal zusätzlich zu den detaillierten Anweisungen in diesem Handbuch ein sicheres Arbeitssystem einsetzen.
3. Mit Ausnahme der Teile, deren Wartungsverfahren in diesem Handbuch beschrieben sind, enthält dieses Gerät keine weiteren Teile, die vom Benutzer gewartet werden können. Das Entfernen von Abdeckungen und Versuche von hierfür unqualifiziertem Personal, Anpassungen oder Wartungsarbeiten durchzuführen, haben zur Folge, dass die Garantie verfällt und können zusätzliche Reparaturkosten auslösen.
4. Es ist jederzeit auf die sicherheitsrelevanten Daten sämtlicher verwendeter Chemikalien Bezug zu nehmen. Allgemein anerkannte Labormethoden zum sicheren Umgang mit Chemikalien sollten eingesetzt werden.
5. Besteht der Verdacht, dass die Sicherheitsvorrichtungen in irgendeiner Weise beschädigt wurden, muss das Gerät außer Betrieb genommen und gegen weiteren Gebrauch gesichert werden. Die Störung sollte der zuständigen Serviceeinrichtung unverzüglich gemeldet werden.

Leggere attentamente queste istruzioni prima di installare o utilizzare il dispositivo.

1. L'unità descritta nel presente manuale è stata realizzata per essere utilizzata solo da personale che ha ricevuto l'apposita formazione. Qualsiasi operazione di regolazione, manutenzione e riparazione deve essere effettuata sulla base di quanto indicato nel presente manuale da personale qualificato consapevole dei rischi connessi.
2. È fondamentale che il personale operativo e il personale addetto alla manutenzione utilizzino un sistema di lavoro sicuro, oltre a seguire le istruzioni specificate nel presente manuale.
3. Oltre a quelli indicati nelle procedure di manutenzione, all'interno di questo dispositivo non sono presenti altri elementi sui quali è possibile effettuare interventi. La rimozione delle protezioni e qualsiasi tentativo di regolazione o di manutenzione posto in essere da personale non qualificato invaliderà la garanzia. In questi casi, sarà necessario pagare un importo per le riparazioni effettuate.
4. È sempre necessario fare riferimento ai dati sulla salute e sulla sicurezza forniti con le sostanze chimiche utilizzate. Adottare le procedure di laboratorio generalmente accettate per la gestione delle sostanze chimiche.

5. Nel caso in cui si sospetti che la salute possa essere pregiudicata in qualsiasi modo, disattivare l'unità per renderla inutilizzabile. Qualsiasi condizione di errore deve essere immediatamente segnalata al responsabile per la manutenzione.

Lea esta información atentamente antes de instalar o utilizar este equipo.

1. La unidad descrita en este manual está diseñada para que solamente la utilice personal con formación. Cualquier operación de ajuste, mantenimiento y reparación debe llevarse a cabo del modo indicado en este manual y debe realizarla una persona cualificada que sea consciente de los peligros que implica.
2. Es fundamental que tanto los operarios como el personal de servicio utilicen un sistema de trabajo seguro, así como las instrucciones detalladas que se especifican en este manual.
3. Cualquier elemento que no se encuentre entre los definidos en los procedimientos de mantenimiento aquí descritos no podrá utilizarse en este instrumento. La extracción de las tapas y los intentos de ajuste o reparación por parte de personal no cualificado invalidarán la garantía y pueden incurrir en cargos adicionales por reparación.
4. Siempre deberían consultarse los datos sobre Salud y Seguridad que se suministran con cualquier producto químico que se utilice. Es necesario llevar a cabo los procedimientos de laboratorio de aceptación generalizada para la manipulación segura de productos químicos.
5. Si existe la sospecha de que las medidas protectoras de seguridad han quedado dañadas en cualquier modo, la unidad debe inutilizarse y protegerse contra toda operación que se intente llevar a cabo. El estado de fallo debe comunicarse inmediatamente a la autoridad de servicio de mantenimiento y reparación pertinente.

Contents

SECTION 1 - INTRODUCTION.....	7
1.1 MICRO VOLUME ACCESSORY DESCRIPTION	7
1.2 GENOVA NANO WITH MICRO VOLUME ACCESSORY SPECIFICATION	7
1.3 UNPACKING.....	8
SECTION 2 – ACCESSORY LAYOUT AND INSTALLATION	9
2.1 ACCESSORY LAYOUT	9
2.2 ACCESSORY REMOVAL.....	9
2.3 ACCESSORY INSTALLATION.....	11
2.4 INITIALISATION	11
SECTION 3 – ACCESSORY SETTINGS.....	13
3.1 ACCESSING THE MICRO VOLUME ACCESSORY SETTINGS	13
3.2 PATH LENGTH SELECTION	14
3.2.1 Known Path Length Measurements	14
3.2.2 Unknown Path Length Measurements	14
3.2.3 Auto Path Length Availability.....	14
SECTION 4 – PERFORMING MICRO VOLUME MEASUREMENTS.....	15
4.1 PIPETTING SAMPLES ONTO THE MICRO VOLUME READ HEAD.....	15
4.2 SAMPLE RECOVERY OR REMOVAL.....	16
SECTION 5 – TOP 10 TIPS FOR SAMPLE MEASUREMENT.....	17
SECTION 6 – STEP BY STEP GUIDE TO MAKING A DNA MEASUREMENT.....	18
6.1 dsDNA Mode	18
6.2 A260/280 Mode	18
6.3 Multi-wavelength Mode.....	19
SECTION 7 – CALIBRATION OF THE MICRO VOLUME ACCESSORY	20
7.1 CALIBRATION SOLUTIONS (035 092)	20
7.2 ACCESSORY CALIBRATION PROCEDURE	20
7.2.1 Micro Volume Accessory Settings	20
7.2.2 Calibration Standard - Data Entry.....	20
7.2.3 Accessory Calibration and Verification	21
SECTION 8 – CLEANING AND DECONTAMINATION.....	24
8.1 ACCESSORY CLEANING	24
8.2 ACCESSORY DECONTAMINATION	24
8.3 READ HEAD RECONDITIONING	24
SECTION 9 – ACCESSORIES	25
9.1 ACCESSORIES.....	25
SECTION 10 – MAINTENANCE AND SERVICE	25
10.1 ROUTINE MAINTENANCE	25
10.2 SERVICE	25
SECTION 11 – TROUBLESHOOTING	26
11.1 CALIBRATION ERROR CODES	26

11.1.1	Calibration Procedure Error Codes	26
11.1.2	Verification Check Error Codes	26
11.2	TROUBLESHOOTING GUIDE	27
11.3	TECHNICAL SUPPORT	27
SECTION 12 – GLOSSARY OF ICONS		28
SECTION 13 – CHEMICAL COMPATABILITY		29

SECTION 1 - INTRODUCTION

1.1 MICRO VOLUME ACCESSORY DESCRIPTION

The Genova Nano is a UV/visible spectrophotometer dedicated to life science analysis. This spectrophotometer incorporates a micro volume sample measurement accessory that allows sample volumes as low as 0.5µl to be analysed. In addition to the standard measurement modes: photometrics, concentration, multi-wavelength, spectrum scanning, quantitation and kinetics, the Genova Nano spectrophotometer is pre-programmed with methods to determine DNA concentration and purity ratios using wavelengths recorded at 260, 280 and 230nm, with an optional correction at 320nm. In addition there are pre-programmed methods for protein analysis such as the Bradford, Lowry, Biuret, BCA and Direct UV methods.

The micro volume accessory can be removed and replaced with the supplied standard cuvette holder converting the Genova Nano to a standard Genova Plus spectrophotometer. Alternatively any of the other 73 series accessories may also be fitted. This life science spectrophotometer uses icon driven software and has an improved navigation system for easy and intuitive usability.

1.2 GENOVA NANO WITH MICRO VOLUME ACCESSORY SPECIFICATION

Wavelength	
Range	198 to 1000nm
Resolution	1nm
Accuracy	± 2nm
Repeatability	± 0.5nm
Spectral bandwidth	5nm

Photometrics	
Absorbance Range	-0.300 to 2.500A (10mm path length equivalent = -15.0 to 125.0A)
Accuracy	±2% @ 1A
Absorbance Precision	Between 0 and 1A = <0.005, 1 to 2A = 2%, above 2A = 4%.
dsDNA Detection Limit (0.5mm)	2.0 ng/µl
dsDNA Maximum Concentration (0.2mm)	6000 ng/µl
Stray light	<0.5% at 340nm and 220nm

Other	
Weight	7.7kg
Path lengths	0.2mm and 0.5mm
Measurement time	<6.5s
Sample size	0.5 to 5.0µl
Operating Temperature	10 to 40°C
Operating Humidity	0 to 80% non-condensing

1.3 UNPACKING

Please check that the following items are included in the packaging:

- Genova Nano spectrophotometer (737 503)
- 10x10mm cuvette holder (630 204)
- 4GB USB memory stick (019 146)
- Universal power supply 24V, 65W (021 060)
- Calibration standards with certificate (035 092)
- Genova Nano instruction manual (737 555)
- Genova Plus instruction manual (736 505)

The Genova Nano is delivered with the micro volume accessory pre-installed and securely packaged in the spectrophotometers sample chamber.

Note: The protective packaging must be removed before the instrument is first initialised.

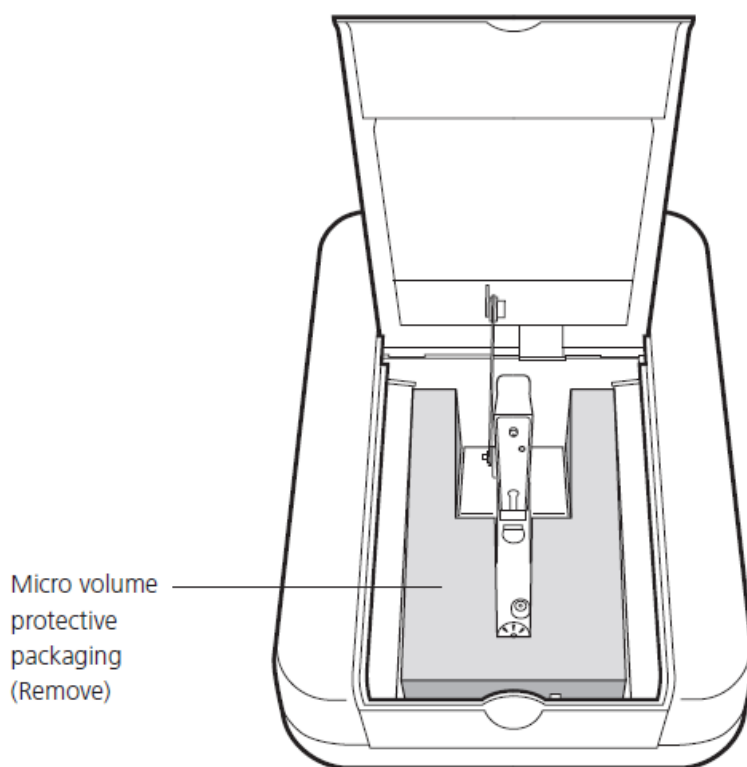


Fig 1.3 – Micro Volume Accessory Unpacking

SECTION 2 – ACCESSORY LAYOUT AND INSTALLATION

2.1 ACCESSORY LAYOUT

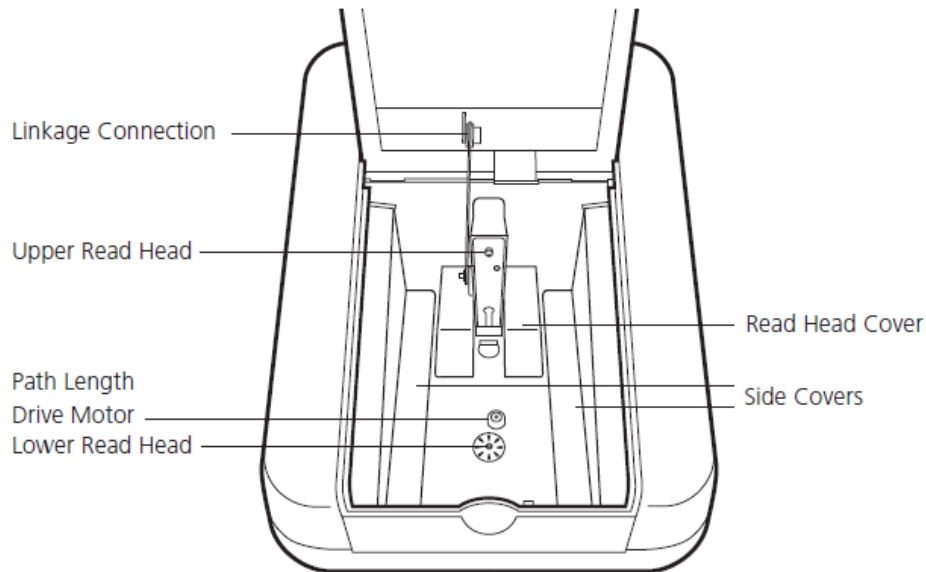



Fig 2.1 – Micro Volume Accessory Layout

2.2 ACCESSORY REMOVAL


The micro volume accessory is pre-installed when purchased as part of the Genova Nano spectrophotometer. The accessory is optically matched to the spectrophotometer in which it is originally installed. Users are therefore advised not to transfer the micro volume accessory to other Genova Plus/Nano spectrophotometers without the assistance of trained service personnel.

The micro volume accessory should not be removed or re-installed un-necessarily as this may affect the accuracy of the optical alignment.


The following steps must be followed to remove and re-install the micro volume accessory into the Genova Nano spectrophotometer.

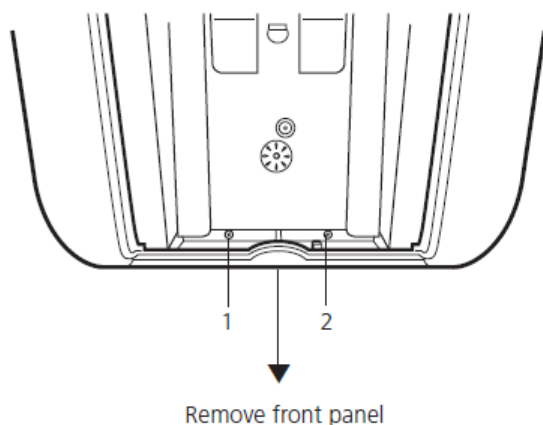

Remove the front panel from the sample chamber by loosening screws 1 and 2 until the front panel can be lifted out in the forward direction.

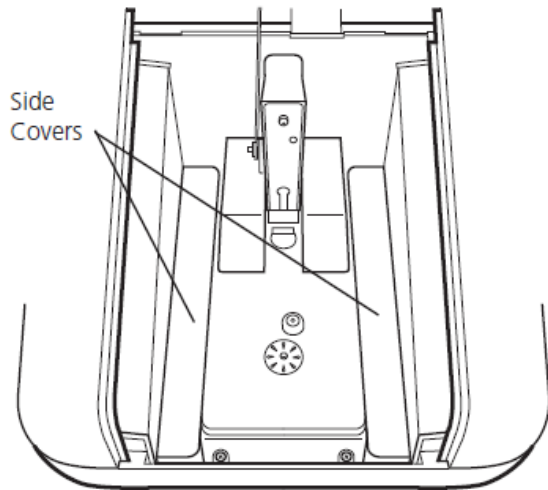


Remove the side covers by lifting them out

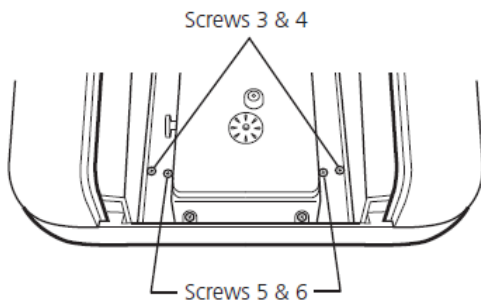


Remove the outer screws 3 and 4.



Ensure that the inner screws 5 and 6 are not adjusted/removed.

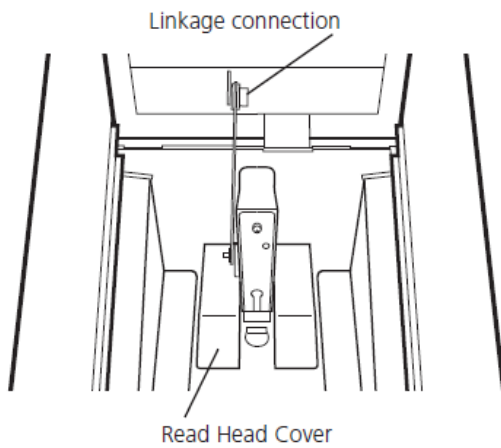


Using the thumb-screw, disconnect the linkage connection from the bracket found on the underside of the spectrophotometer lid and remove the read head cover.

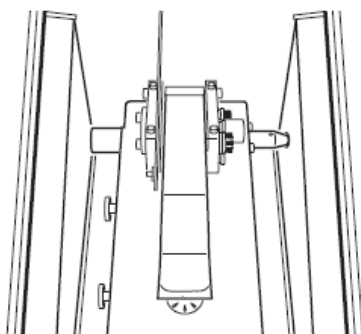

View with linkage disconnected and read head cover removed.

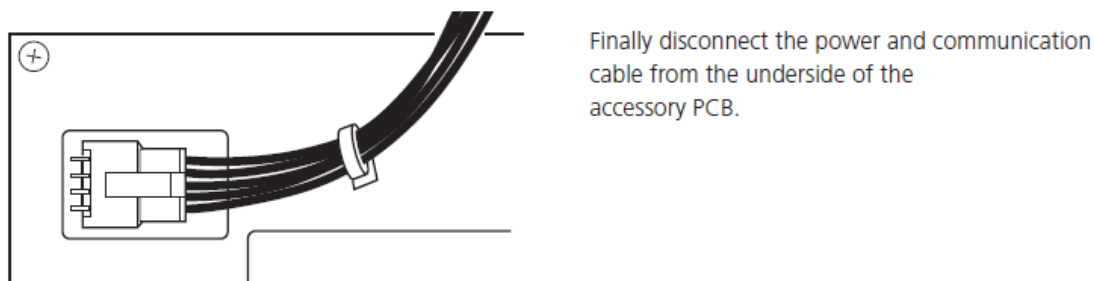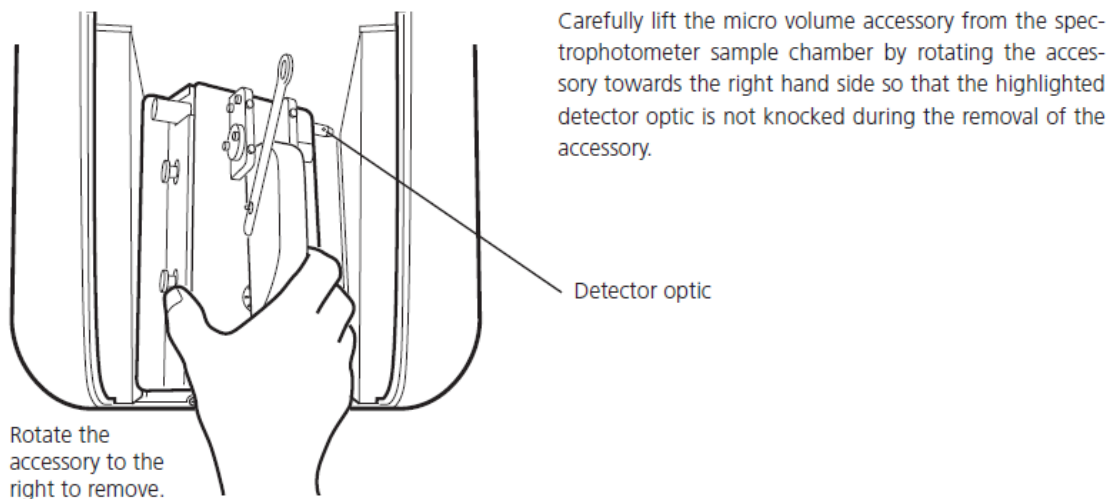

2.3 ACCESSORY INSTALLATION

The micro volume accessory is installed by reversing the procedure described in Section 2.2. Once the accessory has been reinstalled the light intensity passing through the optical system may be checked. See section 3.1 to access the micro volume accessory settings. Press the key adjacent to the Accessory Alignment icon:  When this option is selected, the unit will continually measure and give a display of the level of light passing through the system. Check that the value shown is >60,000. If it is lower than this, please contact service@bibby-scientific.com for further advice.

2.4 INITIALISATION

Connect the power supply unit to the power inlet socket on the rear panel of the instrument and connect to the mains socket. Turn the power on at the mains and switch the instrument on using the power switch on the rear of the instrument.

The instrument will initially check for firmware updates and then perform several power-on tests before displaying the main menu:

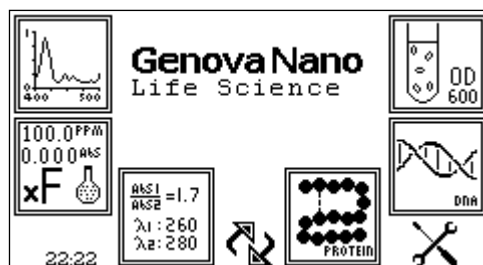


Fig 2.2 – Genova Nano Main Menu

Note: The instrument will return to the last main menu used.

SECTION 3 – ACCESSORY SETTINGS

3.1 ACCESSING THE MICRO VOLUME ACCESSORY SETTINGS

When installed, the micro volume accessory icon is displayed in the bottom right hand corner of the screen in each measurement mode.

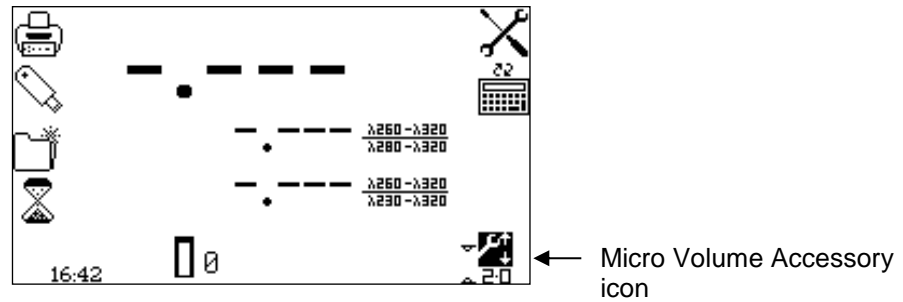


Fig 3.1 – Accessing the Micro Volume Accessory Settings Menu

The micro volume accessory settings are accessed by pressing the key below the micro volume accessory icon.

The micro volume accessory settings allow the user to select the required path length (0.2mm or 0.5mm) for a measurement and to calibrate the accessory using a standard solution with known absorbance values at 260 and 330nm.


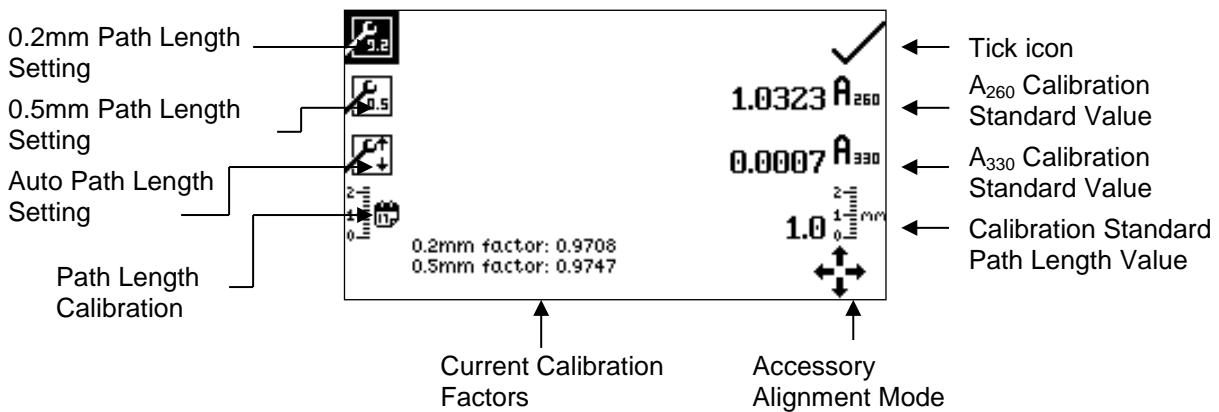


Fig 3.2 – Micro Volume Accessory Settings Menu


3.2 PATH LENGTH SELECTION

3.2.1 Known Path Length Measurements

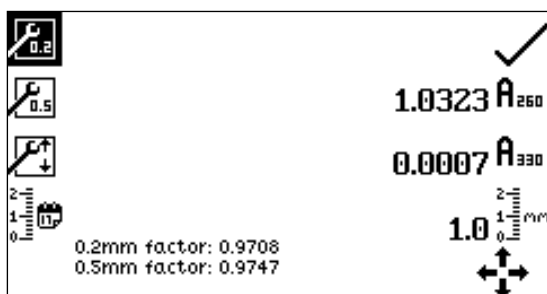

If the required measurement path length is known it can be selected by pressing the button adjacent to the 0.2mm or 0.5mm path length setting icons. The selected setting is indicated by an icon with a black background. Once the required path length setting has been selected press the button adjacent to the tick icon to confirm.

3.2.2 Unknown Path Length Measurements

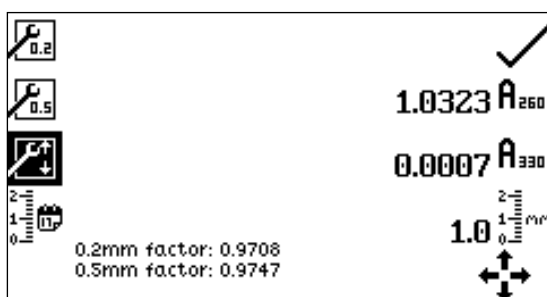

If the required measurement path length is not known in selected modes the auto path length setting can be selected by pressing the button adjacent to the auto path length setting icon. Once the auto path length setting has been selected press the button adjacent to the tick icon to confirm.

The auto path length measurement setting will firstly measure a sample using the 0.5mm path length setting. If the measured photometric value is within range, the value will be displayed on screen and no more measurements are taken. If however the measured value is over-range, the sample will be re-measured using the 0.2mm path length setting.

3.2.3 Auto Path Length Availability

Mode	Auto path length availability
Photometrics	Available
Spectrum, purity scan	Not available
Concentration, concentration plus	Available
Kinetics	Not available
Multi wavelength, multi wavelength plus	Available
Quantitation	Not available
Protein (quantitative assay modes)	Not available
Protein (direct UV)	Available
DNA (all modes)	Available
OD 600	Available


SECTION 4 – PERFORMING MICRO VOLUME MEASUREMENTS

For detailed descriptions of the measurement modes that are available on the Genova Nano spectrophotometer please refer to the supplied Genova Plus operating manual.

4.1 PIPETTING SAMPLES ONTO THE MICRO VOLUME READ HEAD


The Genova Nano spectrophotometer is designed to measure sample volumes ranging from 0.5 μ l to 5.0 μ l.

Jenway recommends that users should, if possible, use at least 2 μ l of sample for their measurements.

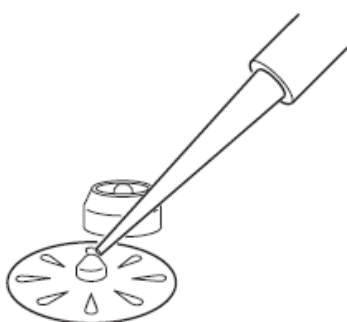


1. With the read head mechanism open, pipette the liquid to be analysed onto the centre of the lower read head. Ensure there are no bubbles in the sample.

Pipetting a sample onto the read head

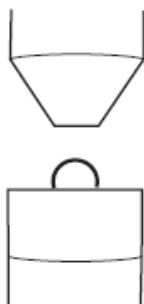

Read head in rest position




Read head in measurement position


2. Close the lid of the spectrophotometer. This will lower the read head assembly down onto the path length drive motor. The upper read head will now be in the rest position, 2mm above the lower read head.
3. When a measurement is initiated, the path length drive motor lowers the upper read head to the specified measurement distance, the photometric measurement is taken and the upper read head is then returned to the rest position.

4.2 SAMPLE RECOVERY OR REMOVAL

Once a measurement is complete, the sample solution can be recovered from the lower read head with a suitable pipette or removed from the read heads by cleaning with a suitable lint free cloth.

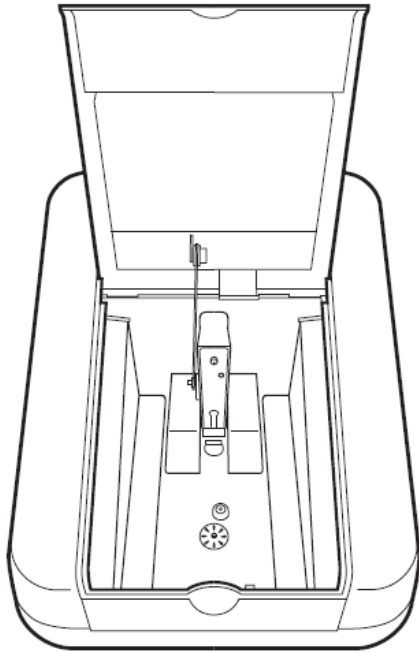

1. Open the lid of the spectrophotometer. The read head mechanism will open to allow access to the upper and lower read heads

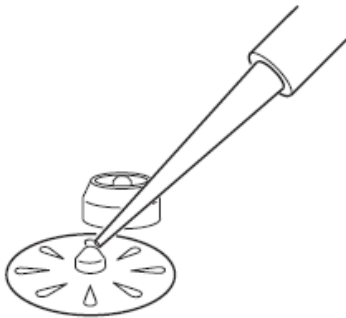

2. The sample can be recovered by carefully drawing the liquid that is retained on the lower read head into a clean pipette tip.
3. Both read heads should then be wiped with a lint free cloth.

4. More rigorous cleaning may be required after the measurement of high concentration samples or samples that pose a contamination risk. See section 8 for further details.

SECTION 5 – TOP 10 TIPS FOR SAMPLE MEASUREMENT





1. Ensure the read heads are clean. Wipe both the upper and lower read heads with a lint-free cloth wetted with deionised water to remove any residues of previous samples. Dry with a fresh cloth.
2. If a stable droplet does not form, “buff” the read head surfaces by rubbing aggressively with a dry laboratory wipe 30-40 times. This will “re-condition” the surface.
3. Make sure that the sample is well mixed and free of air bubbles or particles. If a bubble is created when pipetting the sample, remove the sample and repeat the application.
4. If possible use at least 2µl of sample for measurement. When measuring at 0.2mm path length, a minimum of 0.5µl can be used.
5. Read each sample droplet only once. The read head moves into a default position after the sample has been measured. This means that if the sample is measured a second time, contact of the droplet with the read heads could be lost and the subsequent reading will not give a valid result.
6. Use a sample of sufficient concentration. Remember that the short path length creates a “virtual dilution” of the sample of 1 in 20 at 0.5mm and 1 in 50 at 0.2mm. This means that a sample which would normally read an absorbance of 1.0 in a standard 10mm cuvette will only give a value of 0.05 at 0.5mm or 0.02 at 0.2mm.
7. To minimise any factors which may interfere with a reading such as sample turbidity or contaminants carried over from sample preparation, it is recommended that a background reading is also made at a second reference wavelength (where the absorbance of the sample is very low and unchanging). In the nucleic acid and protein direct UV modes this option is defaulted to ON at a wavelength of 320nm; this can be deactivated if required.
8. Use the same measurement mode if comparing the concentrations of samples. Different modes use different equations to calculate the final sample concentration.
9. Be aware that when measuring micro volume samples, very small changes in absorbance can lead to much greater differences in calculated concentration values due to the inherent “dilution” factor of the small path length. For example, when measuring dsDNA, an absorbance change of just 0.001 equates to a derived concentration change of 1µg/ml at 0.5mm path length (based on 1 A260 unit of dsDNA = 50µg/ml).
10. Jenway recommends that the micro volume accessory is calibrated every 6 months. A set of calibration solutions (Part code 035 092) are supplied with the Genova Nano spectrophotometer for this purpose. Full instructions are given in Section 7.

SECTION 6 – STEP BY STEP GUIDE TO MAKING A DNA MEASUREMENT

The DNA measurement mode of the Genova Nano allows the user to select a method from a list of common nucleic acid measurement tests, including single wavelength concentration measurements for dsDNA, ssDNA, RNA and Oligonucleotides and methods that use absorbance ratios for estimating nucleic acid purity, such as 260nm/280nm and 260nm/230nm. Section 14 of the Genova Plus manual gives further details of the DNA measurement modes.

6.1 dsDNA Mode

This mode simply multiplies the A260 reading by a factor of 50 for dsDNA to calculate the concentration in µg/ml. An additional factor for the path length is also included automatically by the instrument.




1. From the **Life Science** screen select the **DNA mode**:  _{DNA}, followed by **dsDNA**.
2. Press the button next to the **Settings Menu** icon:  and check that the wavelength is set to 260nm, the units are µg/ml and F1 = 50.
3. Lift the lid of the Genova Nano and pipette 2µl of water onto the read head. Close the lid.
Perform the **Blank Reading**: 
4. Lift the lid and wipe the water from both the upper and lower read heads.
5. Pipette 2µl of the DNA sample onto the read head. Close the lid and perform the **Sample Reading**:  F. Record the results.

6.2 A260/280 Mode

This method uses the equation:

$$\text{Concentration } (\mu\text{g/ml}) = (\text{Abs}@260\text{nm} \times 62.9) - (\text{Abs}@280\text{nm} \times 36.0).$$

This equation takes into account any contamination present which may absorb at 280nm (e.g. protein).

1. From the **Life Science** screen select the **DNA mode**:  _{DNA}, followed by **260/280**.
2. Press the button next to the **Settings Menu** icon: . Check that the settings are as follows: Wavelength 1: 260; Wavelength 2: 280; Wavelength 3: 230; units, µg/ml.
3. Touch the button next to the **Calculation Factors** icon:  and check that Factor 1 = 62.9; Factor 2 = 36.0; Sum,=(x_{F1}*A₁)-(x_{F2}*A₂).
4. Press the button next to the **Tick** icon twice to return to the measurement screen.

5. Lift the lid of the Genova Nano and pipette 2µl of water onto the read head. Close the lid. Perform the blank reading.
6. Lift the lid and wipe the water from both the upper and lower read heads.
7. Pipette 2µl of the DNA sample onto the read head. Close the lid and perform the DNA reading. Record the results.



6.3 Multi-wavelength Mode

This mode simply calculates the DNA concentration by multiplying by the factor 50 for dsDNA but also allows correction by a reference wavelength at 320nm.

$$\frac{A_{260}}{A_{280}} = 1.7$$

$$\lambda_1: 260$$


$$\lambda_2: 280$$

1. From the Life Science screen select the **Multiwavelength mode**:
2. Press the button next to the **Settings Menu** icon: . Check that the settings are as follows: Wavelength 1: 260; Wavelength 2: 280; Wavelength 3: 230. Activate the reference Wavelength 4, 320nm. The units are µg/ml.
3. Touch the button next to the **Calculation Factors** icon:  and check that Factor 1 = 50; Factor 2 = 0 and the Sum = (x_{F1}*(A₁-A₄))- (x_{F2}*(A₂-A₄)).
4. Press the button next to the **Tick** icon twice to confirm and return to the measurement screen.
5. Set the path length to 0.5mm. Press the button next to the **Tick** icon to confirm.
6. Lift the lid of the Genova Nano and pipette 2µl of water onto the read head. Close the lid. Perform the blank reading.
7. Lift the lid and wipe the water from both the upper and lower read heads.
8. Pipette 2µl of the DNA sample onto the read head. Close the lid and perform the DNA reading. Record the results.

SECTION 7 – CALIBRATION OF THE MICRO VOLUME ACCESSORY

Jenway recommends that the micro volume accessory is calibrated every 6 months. A set of calibration solutions (Part code 035 092) are supplied with the Genova Nano spectrophotometer.

7.1 CALIBRATION SOLUTIONS (035 092)

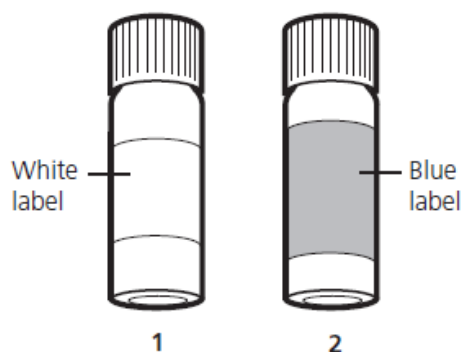


The supplied calibration solution set consists of two vials.

1. Matrix Blank (White)
2. 10x ref - Calibration Standard (Blue)

A calibration certificate is supplied that details the certified absorbance values of the calibration standard and the path length at which these values were determined.


7.2 ACCESSORY CALIBRATION PROCEDURE

7.2.1 Micro Volume Accessory Settings

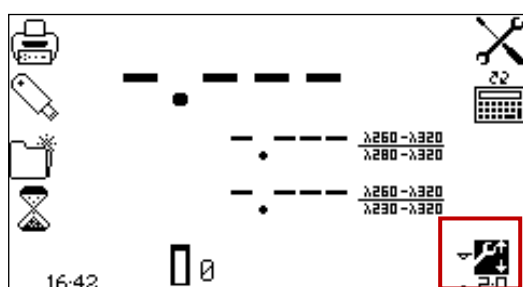


The micro volume accessory settings can be accessed by pressing the key below the **Micro Volume Accessory** icon in any of the Genova Nano's operating modes.


7.2.2 Calibration Standard - Data Entry

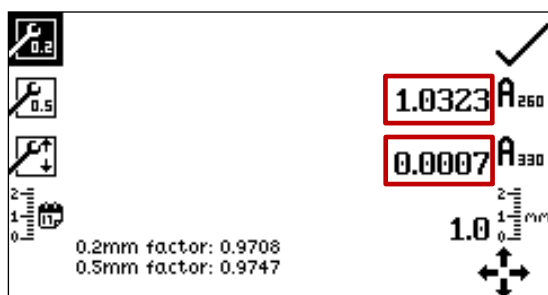

1. Enter the A260 and A330 DNA standard solution values given on the calibration certificate into the accessory settings by pressing the key adjacent to the **Calibration Standard Value** icon.

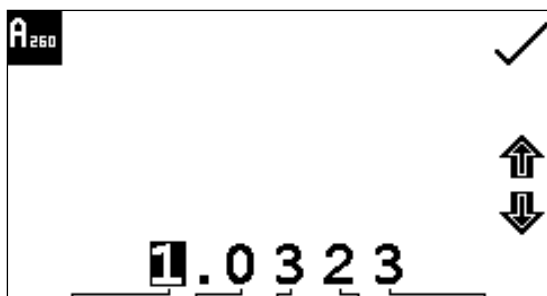

2. Select the digit to be changed using the keys at the bottom of the screen. Use the keys adjacent to the **Arrow** icons to increase or decrease the number. Press the key adjacent to the **Tick** icon to save any changes.

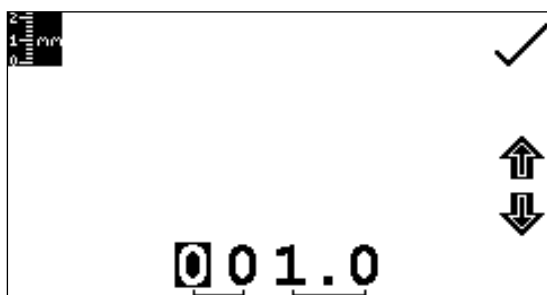


3. Enter the stated path length in mm (1.0mm for the supplied calibration standard solution set) for the DNA standard solution into the accessory settings by pressing the key adjacent to the **Calibration Standard Path Length Value** icon.


4. Select the digit to be changed using the keys at the bottom of the screen. Use the keys adjacent to the **Arrow** icons to increase or decrease the number. Press the key adjacent to the **Tick** icon to save any changes.

7.2.3 Accessory Calibration and Verification

If an error message is displayed during the accessory calibration and verification procedure, refer to Section 11 for further details.

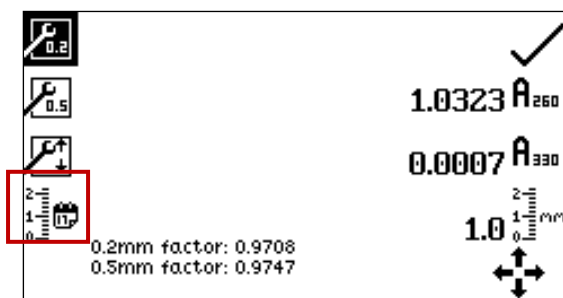


1. The accessory calibration sequence is initiated by pressing the key adjacent to the **Path Length Calibration** icon.

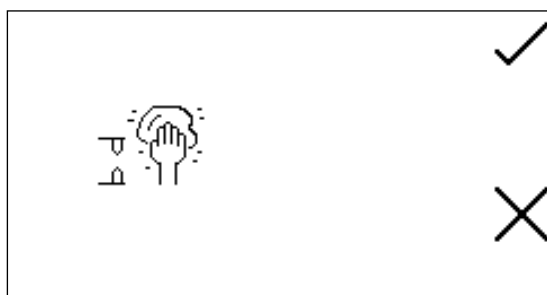

2. The **Air Measurement** icon will be displayed. Use a lint free cloth to clean the upper and lower read heads, close the instrument lid and press the key adjacent to the **Tick** icon to continue. Pressing the key adjacent to the **Cross** icon will return the instrument to the micro volume accessory settings menu screen.


The unit takes five dark and light readings at 260 and 330nm, at both 0.5mm and 0.2mm path lengths.

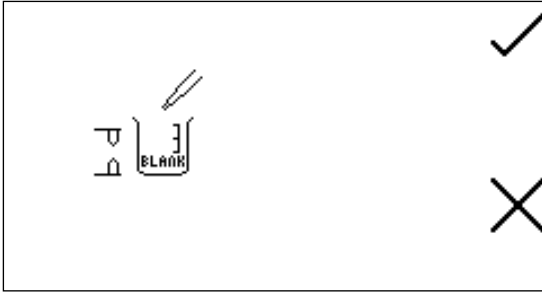

3. The **Blank Solution Measurement** icon will be displayed. Open the instrument lid and pipette a 2.0µl aliquot of the matrix blank solution onto the lower read head. Close the instrument lid and press the key adjacent to the **Tick** icon to initiate the blank measurement.

4. The unit takes five readings at 260 and 330nm, at both 0.5mm and 0.2mm path lengths.

5. If the measured values are within the required tolerances, the **Passes Test** icon will be displayed. Press the button adjacent to the **Tick** icon to continue or the button adjacent to the **Cross** icon to abort the calibration process.

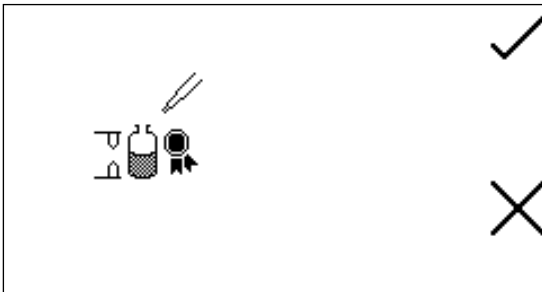


6. The **Calibration Solution Measurement** icon will be displayed. Open the instrument lid and use a lint free cloth to clean the read heads.

7. Pipette a 2.0µl aliquot of the calibration solution onto the lower read head. Close the instrument lid and press the key adjacent to the **Tick** icon to initiate the calibration solution measurement.

8. The unit takes five readings at 260 and 330nm, at both 0.5mm and 0.2mm path lengths.

9. If the measured values are within the required tolerances, the **Passes Test** icon will be displayed. Press the button adjacent to the **Tick** icon to continue or the button adjacent to the **Cross** icon to abort the calibration process.

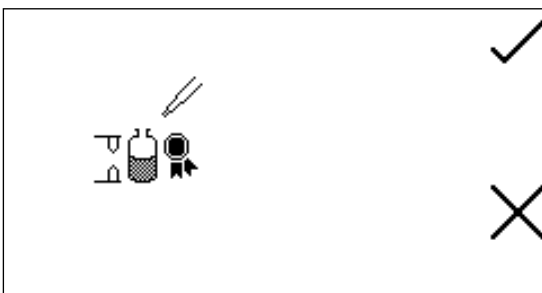


10. The **Calibration Solution Measurement** icon will be displayed for a second time. Open the instrument lid and use a lint free cloth to clean the read heads.

11. Pipette a 2.0µl aliquot of the calibration solution onto the lower read head. Close the instrument lid and press the key adjacent to the **Tick** icon to initiate the calibration solution measurement.

12. The unit takes five readings at 260 and 330nm, at both 0.5mm and 0.2mm path lengths.


13. If the measured values are within the required tolerances, the **Passes Test** icon will be displayed and the instrument will calculate the new path length calibration factors. Press the button adjacent to the **Tick** icon to continue or the button adjacent to the **Cross** icon to abort the calibration process.

14. The new calibration factor values must now be verified by re-measuring the air, blank and standard values.

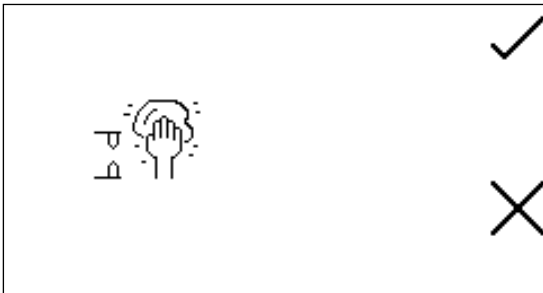

15. The **Air Measurement** icon will be displayed. Open the instrument lid and use a lint free cloth to clean the read heads. Close the instrument lid and press the key adjacent to the **Tick** icon to initiate the blank measurement.


16. The unit takes three dark and light readings at 260 and 330nm, at both 0.5mm and 0.2mm path lengths.

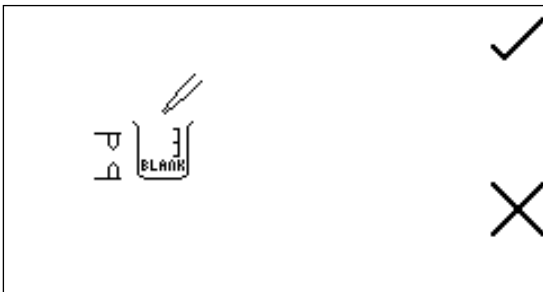

17. The **Blank Solution Measurement** icon will be displayed. Open the instrument lid and pipette a 2.0µl aliquot of the matrix blank solution onto the lower read head. Close the instrument lid and press the key adjacent to the **Tick** icon to initiate the blank measurement.

18. The unit takes three readings at 260 and 330nm, at both 0.5mm and 0.2mm path lengths.


19. If the measured values are within the required tolerances, the **Passes Test** icon will be displayed. Press the button adjacent to the **Tick** icon to continue or the button adjacent to the **Cross** icon to abort the calibration process.

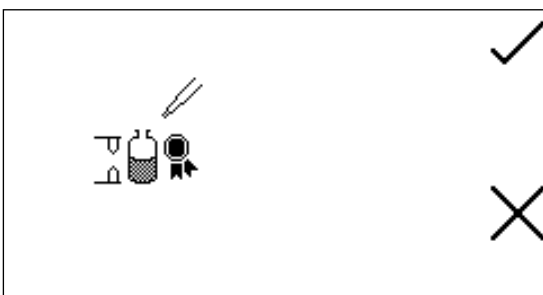

20. The **Calibration Solution Measurement** icon will be displayed. Open the instrument lid and use a lint free cloth to clean the read heads. Open the instrument lid and pipette a 2.0µl aliquot of the calibration solution onto the lower read head. Close the instrument lid and press the key adjacent to the **Tick** icon to initiate the calibration solution measurement.

21. The unit takes three readings at 260 and 330nm, at both 0.5mm and 0.2mm path lengths.

22. If the measured values are within the required tolerances, the **Passes Test** icon will be displayed. Press the button adjacent to the **Tick** icon to continue or the button adjacent to the **Cross** icon to abort the calibration process

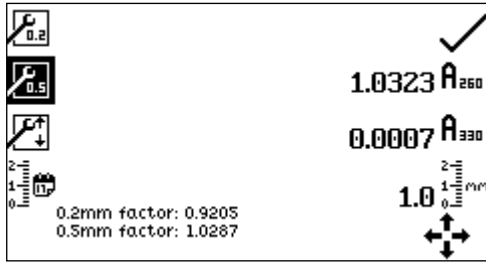

23. Following successful calibration, the instrument display will return to the micro volume accessory settings screen and the new path length calibration factors will be shown.

SECTION 8 – CLEANING AND DECONTAMINATION

8.1 ACCESSORY CLEANING

Wiping the sample from both the upper and lower read heads upon completion of each sample measurement with a lint free cloth is usually sufficient to prevent sample carryover and avoid residue buildup. Although generally not necessary, water aliquots can be used to clean the measurement surfaces after the measurement of particularly highly concentrated samples to ensure no residual sample is retained on either read head. After measuring a large number of samples, it is recommended that the areas around the upper and lower pedestals are cleaned thoroughly. This will prevent spread of contamination from previous samples onto the measurement pedestals which could affect subsequent low-level measurements. A final cleaning of all surfaces with deionised water is also recommended after the last measurement.

8.2 ACCESSORY DECONTAMINATION

If decontamination is necessary, a sanitising solution, such as a 0.5% solution of sodium hypochlorite (1:10 dilution of common commercial bleach solutions – freshly prepared), can be used to ensure that no biologically active material is present on the measurement read heads. The read head fittings are made from stainless steel and are resistant to most common laboratory solvents. See Section 13 - Chemical Compatibility for full details.

8.3 READ HEAD RECONDITIONING

Reagents containing surfactants can “un-condition” the measurement read head surfaces so that the liquid does not form a stable sample droplet. If this occurs, “buff” the read head surfaces by rubbing each measurement surface aggressively with a dry laboratory wipe 30-40 times. This will “re-condition” the surface allowing the sample droplet to form.

SECTION 9 – ACCESSORIES

9.1 ACCESSORIES

Part Code	Description
035 092	Calibration solution set

SECTION 10 – MAINTENANCE AND SERVICE

10.1 ROUTINE MAINTENANCE

Ensure the external surfaces of the unit are clean and free from dust. The sample area should always be kept clean and any accidental spillage should be wiped away immediately.

10.2 SERVICE

Our dedicated service team are on hand to help in the unlikely event that your Jenway equipment develops a fault. Please contact them by one of the following means stating the serial number of the unit and a clear description of the problem:

E-mail: service@bibby-scientific.com

Tel: +44 (0) 1785 810475

On occasion it may be necessary for your equipment to be sent back to our Service Department for repair. In this case please contact the Service Department for a reference number which you should include with your faulty equipment. Please also ensure you include a clear description of the fault and a completed copy of our Decontamination Certificate. This is available as a downloadable pdf file at www.jenway.com or contact us and we will send a copy to you. Please clearly mark the package for the attention of the Service Department and post to the following address:

Bibby Scientific Ltd
Beacon Road
Stone
Staffordshire
ST15 0SA
United Kingdom

All replacement parts are guaranteed for 1 year and wherever possible, returned equipment is turned around in 10 working days.

SECTION 11 – TROUBLESHOOTING

11.1 CALIBRATION ERROR CODES

If an error code is displayed during calibration it will be accompanied by a **Clipboard** icon and a number to indicate the cause of the error. The first time that an error is displayed, it will be possible to repeat the erroneous measurement. If the same error message is shown after the repeat measurement, the complete calibration process will need to be repeated. The table below shows the error codes:

11.1.1 Calibration Procedure Error Codes

Error Code	Symbol	Issue
1	1	Blank solution reading outside of acceptable range
3	3	Calibration solution reading outside of acceptable range
5	5	Duplicate calibration solution readings outside of acceptable range
7	7	0.2mm path length factor outside of acceptable range
8	8	0.5mm path length factor outside of acceptable range

11.1.2 Verification Check Error Codes

9	9	Blank solution reading outside of acceptable range
11	11	Calibration solution reading outside of acceptable range

11.2 TROUBLESHOOTING GUIDE

Issue	Solution
Unable to achieve zero absorbance or 100% transmittance when calibrating	Ensure that there is not a sample on the micro volume accessories read head. Ensure the instrument lid is closed before and during the calibration. Ensure the lamp is working – if the lamp has failed please request service assistance.
Unable to achieve a reading when measuring a sample	Ensure the correct path length is being used. Ensure the sample isn't so dense so that light is not transmitted through the sample. Ensure the lamp is working.



















11.3 TECHNICAL SUPPORT

Jenway have a dedicated Technical Support team made up of experienced scientists who are on hand to help with any applications advice and questions you may have about our products and how to use them. If you require any technical or application assistance please contact the team at:

E-mail: jenwayhelp@bibby-scientific.com

Phone: +44 (0)1785 810433

SECTION 12 – GLOSSARY OF ICONS

Mode	ICON	Description
Common		Back key
Common		Tick icon - Done/yes
Common		Cross icon – Cancel/no
Common		Arrow icon – Move down, decrease
Common		Arrow icon – Move up, increase
Settings		0.2mm path length setting / selected
Settings		0.5mm path length setting / selected
Settings		Auto path length setting / selected
Settings		Path length calibration
Settings		260nm Calibration standard absorbance value
Settings		330nm Calibration standard absorbance value
Settings		Calibration standard path length value
Settings		Micro volume accessory alignment
Calibration		Air measurement
Calibration		Blank solution measurement
Calibration		Calibration solution measurement
Calibration		Passes test
Calibration		Fails test

SECTION 13 – CHEMICAL COMPATABILITY

Assay	Chemical	Concentration
BCA	Sodium bicinchoninate	1%*
BCA	Sodium carbonate	2%*
BCA	Sodium tartrate	0.16%*
BCA	Sodium hydroxide	0.1M*
BCA	Sodium bicarbonate	0.95%*
BCA	Copper (II) sulphate	0.08%
Biuret	Sodium potassium tartrate	0.9%*
Biuret	Copper (II) sulphate	0.3%*
Biuret	Potassium iodide	0.5%*
Biuret	Sodium hydroxide	0.08M
Lowry	Sodium carbonate	1.6%
Lowry	Copper (II) sulphate	0.032%
Lowry	Sodium potassium tartrate	0.016%
Lowry	Sodium dodecyl sulphate	0.08%
Lowry	Sodium hydroxide	0.08M
Lowry	Folin reagent (lithium and sodium molybdotungstophosphate solution)	0.04N*
Bradford	Coomassie brilliant Blue G-250	0.01%*
Bradford	Ethanol	4.75%*
Bradford	Phosphoric acid	8.5%*
Bradford	Sodium hydroxide	0.1M
	DMSO	10%
	Acetonitrile	OK
	Methanol	OK
	2-Propanol	OK

*Highest concentration